


测量详细信息	
Sample Name	Average of '0-0.25B'

测量详细信息	
Measurement Date Time	2021/5/11 18:50:45
Result Source	Averaged

分析	
Particle Name	Diamond
Particle Refractive Index	2.418
Particle Absorption Index	0.010
Dispersant Name	Water
Dispersant Refractive Index	1.330
Scattering Model	Mie
Analysis Model	General Purpose
Weighted Residual	2.14 %
Laser Obscuration	4.83 %

结果	
Span	2.041
Uniformity	0.629
Specific Surface Area	154000 m ² /kg
D [3,2]	0.0390 μm
D [4,3]	0.0608 μm
Dv (5)	0.0158 μm
Dv (10)	0.0194 μm
Dv (50)	0.0491 μm
Dv (90)	0.120 μm
Dv (95)	0.145 μm

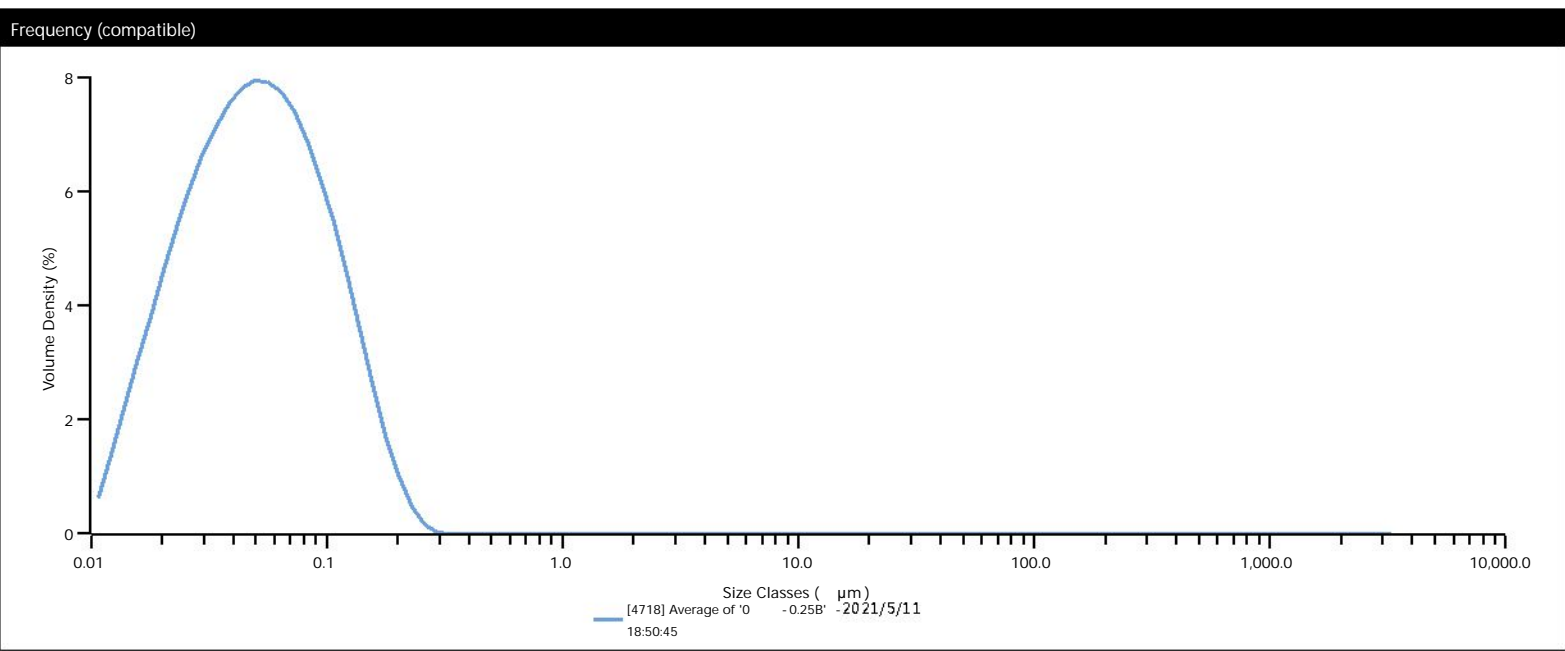

Result											
Size (μm)	% Volume In	Size (μm)	% Volume In	Size (μm)	% Volume In	Size (μm)	% Volume In	Size (μm)	% Volume In	Size (μm)	% Volume In
0.0100	0.52	0.0876	5.21	0.767	0.00	6.72	0.00	58.9	0.00	516	0.00
0.0114	1.15	0.0995	4.55	0.872	0.00	7.64	0.00	66.9	0.00	586	0.00
0.0129	1.83	0.113	3.80	0.991	0.00	8.68	0.00	76.0	0.00	666	0.00
0.0147	2.51	0.128	2.99	1.13	0.00	9.86	0.00	86.4	0.00	756	0.00
0.0167	3.19	0.146	2.18	1.28	0.00	11.2	0.00	98.1	0.00	859	0.00
0.0189	3.85	0.166	1.43	1.45	0.00	12.7	0.00	111	0.00	976	0.00
0.0215	4.47	0.188	0.81	1.65	0.00	14.5	0.00	127	0.00	1110	0.00
0.0244	5.04	0.214	0.37	1.88	0.00	16.4	0.00	144	0.00	1260	0.00
0.0278	5.54	0.243	0.12	2.13	0.00	18.7	0.00	163	0.00	1430	0.00
0.0315	5.96	0.276	0.00	2.42	0.00	21.2	0.00	186	0.00	1630	0.00
0.0358	6.29	0.314	0.00	2.75	0.00	24.1	0.00	211	0.00	1850	0.00
0.0407	6.52	0.357	0.00	3.12	0.00	27.4	0.00	240	0.00	2100	0.00
0.0463	6.63	0.405	0.00	3.55	0.00	31.1	0.00	272	0.00	2390	0.00
0.0526	6.61	0.460	0.00	4.03	0.00	35.3	0.00	310	0.00	2710	0.00
0.0597	6.47	0.523	0.00	4.58	0.00	40.1	0.00	352	0.00	3080	0.00
0.0679	6.18	0.594	0.00	5.21	0.00	45.6	0.00	400	0.00	3500	0.00
0.0771	5.76	0.675	0.00	5.92	0.00	51.8	0.00	454	0.00		