



百特纳米粒度电位分析仪

体积分布报告页

V4.00

样品名称: 0-0.25UM-3	样品来源: YP
检测人员:	检测单位: 河南省亚龙超硬材料有限公司
SOP名称: manual.sop	测试日期: 2024/2/23
备注: Z-均粒径为真实测量数值, 典型值为模拟数值, 仅供参考	测试时间: 9:45


分散介质: 水	样品材质: 聚苯乙烯乳球	检测角度: 90°	子测试次数: 14
温度: 25 °C	折射率: 1.59	平均光强: 415.50 kcps	衰减片编号: 4
粘度: 0.8936 mPa.s(cP)	吸收率: 0.01	分析模型: 通用	样品池种类: PS样品池
折射率: 1.33	激光波长: 671 nm	平衡时间: 120 s	检测点位置: 5 mm

测试结果	均径(d.nm)	面积(%)	峰标准差(nm)	CV (%)
Z-均粒径: 195.05 nm	峰1 135.27	100.00	47.01	34.76
PDI: 0.183	峰2			
截距: 0.73	峰3			

粒径(d.nm)	区间(%)	累积(%)
0.30	0.00	0.00
0.35	0.00	0.00
0.41	0.00	0.00
0.48	0.00	0.00
0.56	0.00	0.00
0.66	0.00	0.00
0.77	0.00	0.00
0.90	0.00	0.00
1.05	0.00	0.00
1.23	0.00	0.00
1.44	0.00	0.00
1.68	0.00	0.00
1.97	0.00	0.00
2.30	0.00	0.00
2.69	0.00	0.00
3.15	0.00	0.00
3.69	0.00	0.00
4.31	0.00	0.00
5.05	0.00	0.00
5.90	0.00	0.00
6.90	0.00	0.00
8.08	0.00	0.00
9.45	0.00	0.00
11.05	0.00	0.00

粒径(d.nm)	区间(%)	累积(%)
12.93	0.00	0.00
15.12	0.00	0.00
17.69	0.00	0.00
20.69	0.00	0.00
24.21	0.00	0.00
28.32	0.00	0.00
33.12	0.00	0.00
38.75	0.00	0.00
45.33	0.00	0.00
53.02	0.00	0.00
62.02	0.00	0.00
72.55	3.53	3.53
84.87	10.72	14.25
99.28	17.17	31.42
116.13	19.56	50.98
135.85	17.74	68.72
158.91	13.49	82.20
185.89	8.82	91.03
217.45	5.02	96.04
254.37	2.47	98.51
297.55	1.03	99.54
348.07	0.35	99.90
407.16	0.09	99.99
476.29	0.01	100.00

粒径(d.nm)	区间(%)	累积(%)
557.15	0.00	100.00
651.73	0.00	100.00
762.38	0.00	100.00
891.81	0.00	100.00
1043.22	0.00	100.00
1220.32	0.00	100.00
1427.50	0.00	100.00
1669.85	0.00	100.00
1953.34	0.00	100.00
2284.96	0.00	100.00
2672.88	0.00	100.00
3126.66	0.00	100.00
3657.48	0.00	100.00
4278.42	0.00	100.00
5004.77	0.00	100.00
5854.44	0.00	100.00
6848.35	0.00	100.00
8011.01	0.00	100.00
9371.05	0.00	100.00
10961.99	0.00	100.00
12823.02	0.00	100.00
15000.00	0.00	100.00

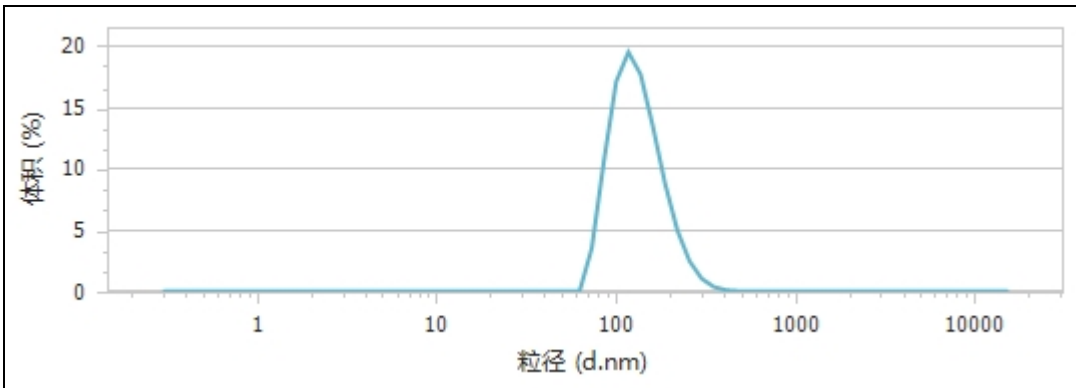

典型值	粒径(d.nm)
D10	79.99
D20	89.70
D30	98.09
D40	106.67
D50	115.29
D60	126.16
D70	138.04
D80	155.15
D90	182.76
D100	12823.02